

# TSX<sup>®</sup>

## Implant System






# Table of Contents

<b>Implants</b>	<b>3</b>
TSX Implants	3
<b>Healing Components</b>	<b>4</b>
Healing Collar Selection Guidelines	4
Encode® Healing Abutments	4
Healing Collars	5
<b>Restorative Solutions</b>	<b>6</b>
Traditional Impression Transfer	6
Provisional Restorations	7
Digital Restorations	8
Cement-Retained Restorations	9
“Cast-To” Gold Restorations	13
Screw-Retained Restorations	14
OverdenSURE® Removable Attachment System	17
Prosthetic Tools	20
<b>Surgical Kit and Instrumentation</b>	<b>22</b>
Instrument Kit System Overview	22
Tapered Screw-Vent Surgical Kit	24
Dríva™ Gold Series Surgical Drills	26
Guided Surgery Instrumentation	29
Drill Stop Kit	31
Bone Profilers	32

# Implants


## TSX Implant

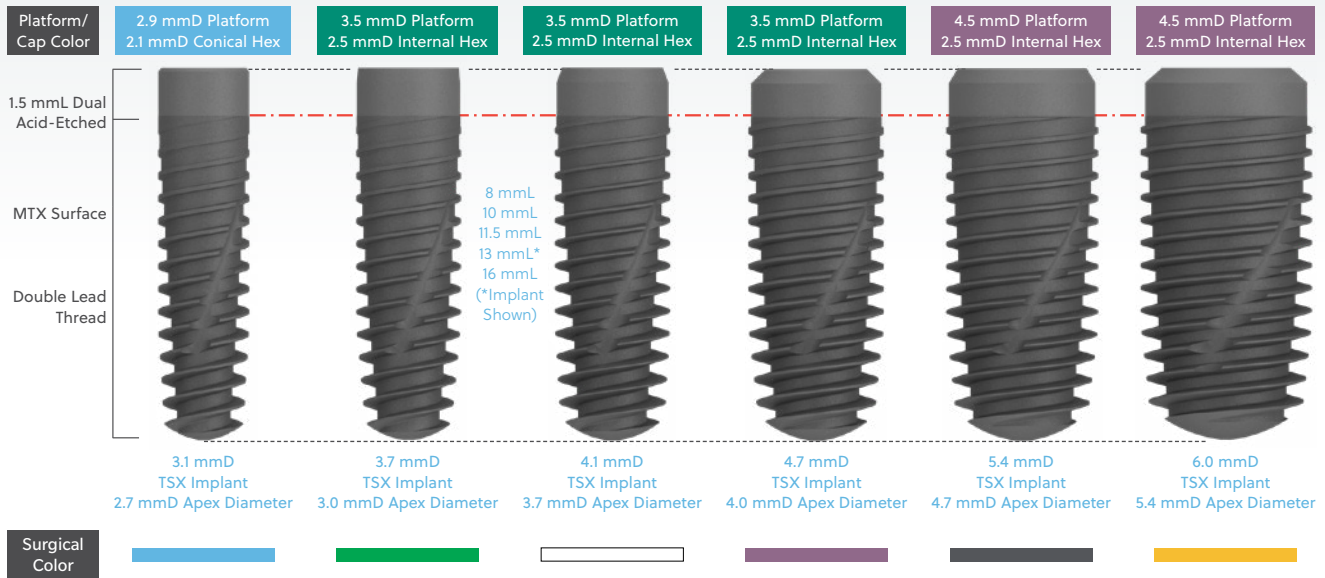

## Surgical Cover Screws

Included with Implant.


Implant Platform		
● NP (2.9 mmD)	● 3.5 mmD	● 4.5 mmD
CCSNP	TSC	TSCW



## TSX Implants

Includes cover screw and optional alignment pin to aid in guiding parallelism during multiple implant placement.

Implant Diameter	Implant Platform	Internal Hex Connection	Implant Length				
			8 mmL	10 mmL	11.5 mmL	13 mmL	16 mmL
3.1 mmD	● 2.9 mmD	2.1 mmD	TSX31B8	TSX31B10	TSX31B11	TSX31B13	TSX31B16
3.7 mmD	● 3.5 mmD	2.5 mmD	TSX37B8	TSX37B10	TSX37B11	TSX37B13	TSX37B16
4.1 mmD	● 3.5 mmD	2.5 mmD	TSX41B8	TSX41B10	TSX41B11	TSX41B13	TSX41B16
4.7 mmD*	● 3.5 mmD	2.5 mmD	TSX47B8	TSX47B10	TSX47B11	TSX47B13	TSX47B16
5.4 mmD	● 4.5 mmD	2.5 mmD	TSX54B8	TSX54B10	TSX54B11	TSX54B13	TSX54B16
6.0 mmD*	● 4.5 mmD	2.5 mmD	TSX6B8	TSX6B10	TSX6B11	TSX6B13	TSX6B16




\*Note: The 4.7 mmD implant features a green color-coded 3.5 mmD platform and the 6.0 mmD implant has a purple color-coded 4.5 mmD platform, unlike TSV® Implants.

# Healing Components

## Healing Collar Selection Guidelines

### Selecting a Healing Collar:

- Determine the size of the implant platform
- Select the emergence profile that best suits the site being restored. The profile should match the transfer and/or abutment to be used
- Select the cuff height so that the top of the component protrudes slightly above the surrounding tissue



HC3/TEHA3/TEEHA3 = 3.5 mmD (Implant Platform) Healing Collar  
 HC4/TEHA4/TEEHA4 = 4.5 mmD (Implant Platform) Healing Collar

### Example:

TEEHA333 = 3.5 mmD (Implant Platform) Healing Abutment, 3.8 mmD Emergence Profile, 3.0 mm Cuff Height (middle digit equals profile, last digit equals height)  
 TEHA3383 = 3.5 mmD (Implant Platform) Healing Abutment, 3.8 mmD Emergence Profile, 3.0 mm Cuff Height (middle two digits equals profile, last digit equals height)  
 HC343 = 3.5 mmD (Implant Platform) Healing Collar, 4.5 mmD Emergence Profile, 3.0 mm Cuff Height (second digit equals profile, third digit equals height)

### Encode Emergence Healing Abutments\*

Encode Healing Abutment is a 3-in-1 two-piece healing abutment/impression coping/scan-body.

Implant Platform	Emergence Profile	Cuff Height		
		3.0 mm	5.0 mm	7.0 mm
● 3.5 mmD	3.8 mmD	TEEHA333	TEEHA335	TEEHA337
● 3.5 mmD	5.0 mmD	TEEHA353	TEEHA355	TEEHA357
● 3.5 mmD	6.5 mmD	TEEHA363	TEEHA365	TEEHA367
● 4.5 mmD	4.5 mmD	TEEHA443	TEEHA445	TEEHA447
● 4.5 mmD	5.5 mmD	TEEHA453	TEEHA455	TEEHA457
● 4.5 mmD	6.5 mmD	TEEHA463	TEEHA465	TEEHA467
● 4.5 mmD	7.5 mmD	TEEHA473	TEEHA475	TEEHA477



\*Not available in all markets.

### Encode Healing Abutments\*

Encode Healing Abutment is a 3-in-1 two-piece healing abutment/impression coping/scan-body.


Implant Platform	Emergence Profile	Cuff Height		
		3.0 mm	5.0 mm	7.0 mm
● 3.5 mmD	3.8 mmD	TEHA3383	TEHA3385	TEHA3387
● 3.5 mmD	5.0 mmD	TEHA3503	TEHA3505	—
● 4.5 mmD	5.0 mmD	TEHA4503	TEHA4505	—
● 4.5 mmD	5.6 mmD	TEHA4563	TEHA4565	TEHA4567
● 4.5 mmD	6.0 mmD	TEHA4603	TEHA4605	—




\*Not available in all markets.

## Healing Collars

Implant Platform	Emergence Profile	Cuff Height		
		1.5 mm	3.0 mm	4.5 mm
● NP (2.9 mmD)	3.7 mmD	CHCNP31	CHCNP33	CHCNP34
● NP (2.9 mmD)	4.5 mmD	CHCNP41	CHCNP43	CHCNP44

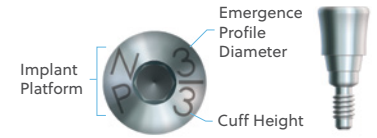

Implant Platform	Emergence Profile	Cuff Height		
		3.0 mm	5.0 mm	7.0 mm
● 3.5 mmD	3.5 mmD (No Flare)	HC333	HC335	—
● 3.5 mmD	4.5 mmD	HC343	HC345	HC347
● 3.5 mmD	5.5 mmD	HC353	HC355	—
● 4.5 mmD	4.5 mmD (No Flare)	HC443	HC445	—
● 4.5 mmD	5.5 mmD	HC453	HC455	HC457
● 4.5 mmD	6.5 mmD	HC463	HC465	—

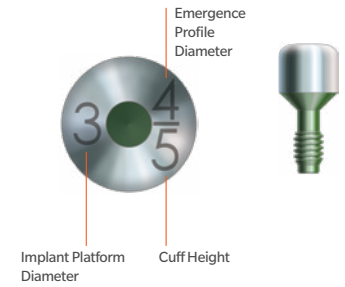

# Restorative Solutions

## Traditional Impression Transfers

### Fixture Mount/Transfers

Not included with TSX Implant. Includes a Retaining Screw (URS2). Can be used as a Preparable Temporary Abutment.

Implant Platform	Emergence Profile	Item No.
● 3.5 mmD	4.5 mmD	FMT3
● 4.5 mmD	5.5 mmD	FMT4
Replacement Retaining Screw	—	URS2



### Indirect Transfers (Closed-Tray Procedure)


Color-coded by implant platform. Includes a Retaining Screw (CASLT).

Implant Platform	Emergence Profile	Cuff Height		
		1.5 mm	3.0 mm	4.5 mm
● NP (2.9 mmD)	3.7 mmD	CITNP31	CITNP33	CITNP34
● NP (2.9 mmD)	4.5 mmD	CITNP41	CITNP43	CITNP44
Replacement Retaining Screw		CASLT	CASLT	CASLT



Color-coded by implant platform. Includes a Retaining Screw (HLTS2).

Implant Platform	Emergence Profile			
	3.5 mmD	4.5 mmD	5.5 mmD	6.5 mmD
● 3.5 mmD	HLT3/3	HLT3/4	HLT3/5	—
● 4.5 mmD	—	HLT4/4	HLT4/5	HLT4/6
3.0 mm Extension Screw for Indirect Transfer	HLTE	HLTE	HLTE	HLTE
Replacement Retaining Screw	HLTS2	HLTS2	HLTS2	HLTS2



### Direct Transfers (Open-Tray Procedure)

Color-coded by implant platform. Includes a Retaining Screw (CASLC).

Implant Platform	Emergence Profile	Cuff Height		
		1.5 mm	3.0 mm	4.5 mm
● NP (2.9 mmD)	3.7 mmD	CDTNP31	CDTNP33	CDTNP34
● NP (2.9 mmD)	4.5 mmD	CDTNP41	CDTNP43	CDTNP44
Replacement Retaining Screw		CASLC	CASLC	CASLC






Color-coded by implant platform. Includes a Retaining Screw (DHTS).

Implant Platform	Emergence Profile			
	3.5 mmD	4.5 mmD	5.5 mmD	6.5 mmD
● 3.5 mmD	DHT3/3	DHT3/4	DHT3/5	—
● 4.5 mmD	—	DHT4/4	DHT4/5	DHT4/6
Replacement Retaining Screw	DHTS	DHTS	DHTS	DHTS



## Titanium Implant Analogs for Stone Models

Color-coded by implant platform.


Implant Platform	Item No.
 NP (2.9 mmD)	CIANP
 3.5 mmD	IA3
 4.5 mmD	IA4



## Provisional Restorations

### Titanium Temporary Abutment



Includes a Retaining Screw (CUAS) and a Long Processing Screw (CASLC).

Implant Platform	Emergence Profile	Item No.
 NP (2.9 mmD)	3.5 mmD	CTANP31
Replacement Retaining Screw		CUAS
Replacement Long Processing Screw		CASLC



### Plastic Temporary Abutments, Straight



Includes Retaining Screw and Processing Screw (DHTS2).

Implant Platform	Emergence Profile	Cuff Height	
		1.0 mm	4.0 mm
 3.5 mmD	4.5 mmD	PT341S	PT344S
 4.5 mmD	5.5 mmD	PT451S	PT454S
Replacement Retaining Screw, Long		DHTS2	DHTS2



### Plastic Temporary Abutments, Angled, 17°



Includes Retaining Screw and Processing Screw (DHTS2).


Implant Platform	Emergence Profile	Cuff Height	
		1.0 mm	4.0 mm
 3.5 mmD	4.5 mmD	PT341A	PT344A
 4.5 mmD	5.5 mmD	PT451A	PT454A
Replacement Retaining Screw, Long		DHTS2	DHTS2



## Digital Restorations

### Express and Flex Ti-Bases


Seating Surface	Express		Flex	
	Hexed	Non-Hexed	Hexed	Non-Hexed
 3.5 mm	TE351	TE352	TF3121	TF3122
 4.5 mm	TE451	TE452	TF4121	TF4122

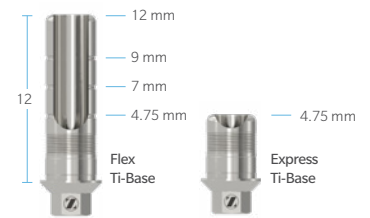

Includes ASC Screw (MHLASC).

### Angled Screw Channel Drivers and Tips for Express and Flex Abutments

Description	Mode of Use	Item No.
Angled Screw Channel Driver, 24 mmL	TWR	TASCD24
Angled Screw Channel Driver, 30 mmL	TWR	TASCD30
Angled Screw Channel Driver Tip, 24 mmL	L-TIRW	TASCT24
Angled Screw Channel Driver Tip, 30 mmL	L-TIRW	TASCT30



### Patient-Specific Abutments

Available in titanium.

Computer-aided design and custom-milled CAD/CAM precision.  
Please contact a ZimVie Dental representative for additional information.

**Note:** Patient-Specific Abutments are only available in select markets.



### Tools and Accessories for Express and Flex Abutments

Description	Item No.
Torque Wrench, Restorative Adjustable torque range 10 Ncm – 35 Ncm	TWR
Low Torque Indicating Ratchet Wrench (Includes C9980 Latchlock Adapter)	L-TIRW
Low Torque Indicating Ratchet Wrench Standard ISO 1797 Latchlock Adapter	C9980
GemLock® Retaining Square Ratchet for Restorative Use with HX1.25, HXL1.25 and SRT	RSR
Express and Flex TSV ASC Screw	MHLASC



### Digital Implant Analogs

Seating Surface	Item No.
3.5 mm	ILATSV35
4.5 mm	ILATSV45







## Cement-Retained Restorations

### Color Coding Chart: Emergence Profile on Hex-Lock Contour and Short Restorative Abutments/Components




Colors correspond to the abutment emergence profile on Hex-Lock® Contour and Short Abutments and related Contour and Short Restorative Components.

Abutment Emergence Profile*	Color-coding
4.5 mmD	 Tan
5.5 mmD	 Rose

\*For Hex-Lock Contour and Short Restorative components.

### Hex-Lock Contour Abutments, Straight







Includes a Retaining Screw (CUAS).

Implant Platform	Emergence Profile	Cuff Height		
		1.5 mm	3.0 mm	4.5 mm
 NP (2.9 mmD)	N/A 3.7 mmD*	CANP31S	CANP33S	CANP34S
 NP (2.9 mmD)	 4.5 mmD*	CANP41S	CANP43S	CANP44S
Replacement Retaining Screw		CUAS	CUAS	CUAS



\*Contour components with 3.7 mmD Emergence Profile are not compatible with 3.5 mmD Contour Restorative Components.



Includes a Retaining Screw (MHLAS).

Implant Platform	Emergence Profile	Cuff Height		
		1.0 mm	2.0 mm	3.0 mm
 3.5 mmD	 4.5 mmD	ZOA341S	ZOA342S	ZOA343S
 4.5 mmD	 4.5 mmD	ZOA441S	ZOA442S	ZOA443S
 4.5 mmD	 5.5 mmD	ZOA451S	ZOA452S	ZOA453S
Replacement Retaining Screw		MHLAS	MHLAS	MHLAS









### Hex-Lock Contour Abutments, Angled 17°

Includes a Retaining Screw (CUASA or CUAS).

Implant Platform	Emergence Profile	Cuff Height	
		1.5 mm	3.0 mm
 NP (2.9 mmD)	3.7 mmD*	CANP31A	CANP33A
 NP (2.9 mmD)	4.5 mmD**	CANP41A	CANP43A
Replacement Retaining Screw		CUASA	CUAS







Includes a Retaining Screw (AH20S).

Implant Platform	Emergence Profile	Cuff Height	
		1.0 mm	2.0 mm
 3.5 mmD	 4.5 mmD	ZOA341A	ZOA342A
 4.5 mmD	 4.5 mmD	ZOA441A	ZOA442A
 4.5 mmD	 5.5 mmD	ZOA451A	ZOA452A
Replacement Retaining Screw		AH20S	AH20S





### Contour Abutment Try-Ins and Try-In Kit

Implant Platform	Emergence Profile	Description	Item No.
 3.5 mmD	 4.5 mmD	Set of 5: Various Angles, Cuff Heights	ZOAT34
 4.5 mmD	 5.5 mmD	Set of 5: Various Angles, Cuff Heights	ZOAT45
All	All	3 Sets of 5: All Sizes	ZOATKIT





### Contour Restorative Kits

Includes 1 Contour Impression Cap, 1 Contour Waxing Coping, 1 Contour Abutment Analog (plastic), 1 Contour Provisional Coping. Choose parts to match the emergence profile of the Hex-Lock Contour Abutment being restored.

Emergence Profile	Straight	17°
 4.5 mmD	ZCRKIT4S	ZCRKIT4A
 5.5 mmD	ZCRKIT5S	ZCRKIT5A





### Contour Provisional Copings

Emergence Profile	Straight	17°
 4.5 mmD	ZCPROV4S	ZCPROV4A
 5.5 mmD	ZCPROV5S	ZCPROV5A





### Contour Impression Caps

Emergence Profile	Straight	17°
 4.5 mmD	ZOCIMP4S	ZOCIMP4A
 5.5 mmD	ZOCIMP5S	ZOCIMP5A





### Contour Abutment Analogs, Titanium

Emergence Profile	Straight	Angled
 4.5 mmD	TCANA4S	TCANA4A
 5.5 mmD	TCANA5S	TCANA5A







### Contour Waxing Copings

Emergence Profile	Straight	17°
 4.5 mmD	ZOCWAX4S	ZOCWAX4A
 5.5 mmD	ZOCWAX5S	ZOCWAX5A



### Hex-Lock Short Abutments



Includes a Retaining Screw (MHLAS).

Implant Platform	Emergence Profile	Cuff Height	
		1.0 mm	2.0 mm
 3.5 mmD	 4.5 mmD	SA341	SA342
 4.5 mmD	 5.5 mmD	SA451	SA452
Replacement Retaining Screw		MHLAS	MHLAS





### Short Restorative Kits

Includes 1 Short Impression Cap, 1 Short Waxing Coping, 1 Short Abutment Analog, 1 Short Provisional Coping. Choose parts to match the emergence profile of the Hex-Lock Short Abutment being restored.

Emergence Profile	Item No.
 4.5 mmD	SARKIT4
 5.5 mmD	SARKIT5





### Short Provisional Copings

Emergence Profile	Item No.
 4.5 mmD	SAPROVP4
 5.5 mmD	SAPROVP5





### Short Impression Caps

Emergence Profile	Item No.
 4.5 mmD	SAIMP4
 5.5 mmD	SAIMP5





### Short Abutment Analogs, Titanium

Emergence Profile	Item No.
 4.5 mmD	SAANA4
 5.5 mmD	SAANA5





### Short Waxing Copings

Emergence Profile	Item No.
 4.5 mmD	SAWAX4
 5.5 mmD	SAWAX5



### Hex-Lock Abutments


Includes a Retaining Screw (MHLAS).

Implant Platform	Emergence Profile			
	3.5 mmD	4.5 mmD	5.5 mmD	6.5 mmD
 3.5 mmD	HLA3/3	HLA3/4	HLA3/5	—
 4.5 mmD	—	HLA4/4	HLA4/5	HLA4/6
Replacement Retaining Screw, Short	MHLAS	MHLAS	MHLAS	MHLAS
Replacement Retaining Screw, Long	HLTS2	HLTS2	HLTS2	HLTS2





### Angled Abutments, 20°

Includes a Retaining Screw (CUAS).

Implant Platform	Emergence Profile	Item No.
 NP (2.9 mmD)	3.5 mmD	C20A3
Replacement Retaining Screw		CUAS



Includes a Retaining Screw (AH2OS).

Implant Platform	Emergence Profile	Item No.
 3.5 mmD	4.5 mmD	AH20/4
 4.5 mmD	5.5 mmD	AH20W/5
Replacement Retaining Screw	—	AH2OS



## "Cast-To" Gold Restorations

### "Cast-To" Gold Abutments, Engaging

Includes a Retaining screw (CUAS).

Implant Platform	Emergence Profile	Item No.
● NP (2.9 mmD)	3.5 mmD	CEANP31
Replacement Retaining Screw		CUAS
Long Processing Screw		CASLC



Includes Retaining Screw (MHLAS).

Implant Platform	Item No.
● 3.5 mmD	HLA3G
● 4.5 mmD	HLA4G
Replacement Retaining Screw	MHLAS
Waxing Screw for "Cast-To" Abutments	MTWSD



### "Cast-To" Gold Abutments, Non-Engaging

Includes Retaining Screw (MHLAS).

Implant Platform	Item No.
● 3.5 mmD	NEA3G
● 4.5 mmD	NEA4G
Replacement Retaining Screw	MHLAS



## Screw-Retained Restorations

### Straight Universal Multi-Unit Abutments

Non-engaging, abutment does not engage in the internal hex connection. Not for use in single unit restorations. Healing Cap (UMUA-HCS) sold separately.

Implant Platform	Collar Height				
	1.0 mm	2.0 mm	3.0 mm	4.0 mm	5.0 mm
● NP (2.9 mmD)	UMUA-NP291S	UMUA-NP292S	UMUA-NP293S	UMUA-NP294S	UMUA-NP295S
● 3.5 mmD	UMUA-TSV351S	UMUA-TSV352S	UMUA-TSV353S	UMUA-TSV354S	UMUA-TSV355S
● 4.5 mmD	UMUA-TSV451S	UMUA-TSV452S	UMUA-TSV453S	UMUA-TSV454S	UMUA-TSV455S



### Angled Universal Multi-Unit Abutments, 17°

Abutments engage internal hex connection. Not for use in single unit (incl. preassembled retaining screw).

Implant Platform	Cuff Height	
	2.5 mm	3.5 mm
● NP (2.9 mmD)	UMUA-NP2925-17S	UMUA-NP2935-17S
● 3.5 mmD	UMUA-TSV3525-17S	UMUA-TSV3535-17S
● 4.5 mmD	UMUA-TSV4525-17S	UMUA-TSV4535-17S



### Angled Universal Multi-Unit Abutments, 30°

Abutments engage internal hex connection. Not for use in single unit (incl. preassembled retaining screw).

Implant Platform	Cuff Height	
	3.5 mm	4.5 mm
● NP (2.9 mmD)	UMUA-NP2935-30S	UMUA-NP2945-30S
● 3.5 mmD	UMUA-TSV3535-30S	UMUA-TSV3545-30S
● 4.5 mmD	UMUA-TSV4535-30S	UMUA-TSV4545-30S



### Universal Abutment Healing Cap

Healing Cap threads onto the Universal Multi-Unit Abutment and Angled Multi-Unit Abutment.

Description	Item No.
Universal Abutment Healing Cap	UMUA-HCS



### Universal Abutment Impression Coping

Impression Coping thread onto the Universal Multi-Unit Abutment and Angled Multi-Unit Abutment for impression-taking. This method transfers the abutment position.

Description	Height	Item No.
Universal Abutment Impression Coping, Open-Tray Includes Transfer Screws	-	UMUA-OTIC
Universal Abutment Impression Coping, Closed-Tray	5 mm	UMUA-CTICS
Universal Abutment Impression Coping, Closed-Tray, (Qty. 4)	5 mm	UMUA-CTICS4
Universal Abutment Impression Coping, Closed-Tray	8 mm	UMUA-CTICL
Universal Abutment Impression Coping, Closed-Tray, (Qty. 4)	8 mm	UMUA-CTICL4



### Universal Abutment Scan Bodies

Scan Body thread onto the Universal Multi-Unit Abutment and Angled Multi-Unit Abutment.

Description	Item No.
Universal Abutment Scan Body, Intraoral	UMUA-SBIO
Universal Abutment Scan Body, Ti-Base, (Qty. 5)	UMUA-SBTB5
Universal Abutment Scan Body, Desktop Includes Multi-Unit Screw (UMUA-S)	UMUA-SBDT



### Universal Abutment Ti-Base

Ti-Base thread onto the Universal Multi-Unit Abutment and Angled Multi-Unit Abutment.

Description	Height	Item No.
<b>Universal Abutment Ti-Base</b> Includes Multi-Unit Screw (UMUA-S)	6 mm	UMUA-TTS
<b>Universal Abutment Ti-Base</b> Includes Multi-Unit Screw (UMUA-S)	8 mm	UMUA-TTL



### Universal Abutment Angulated Screw Channel Ti-Base

Description	Item No.
<b>Universal Abutment Angulated Screw Channel Ti-Base</b> Includes Angulated Screw Channel Screw (UMUA-ASCTS)	UMUA-ASCT



### Universal Abutment Analog for Stone Models

Description	Item No.
<b>Universal Abutment Analog</b>	UMUA-A



### Universal Abutment Digital Analog

Description	Item No.
<b>Universal Abutment Digital Analog</b> Includes Multi-Unit Screw (UMUA-S)	UMUA-DA



### Replacement Screws for Universal Multi-Unit Components

Description	Item No.
<b>Universal Multi-Unit Screw</b>	UMUA-S
<b>Universal Angulated Screw Channel Screw</b>	UMUA-ASCTS



### Universal Abutment Temporary Cylinder

Temporary Cylinder threads onto the Universal Multi-Unit Abutment and Angled Multi-Unit Abutment.

Description	Item No.
<b>Universal Abutment Temporary Cylinder</b> Includes Multi-Unit Screw (UMUA-S)	UMUA-TCS



### Universal Abutment OverdenSURE® Attachment

Description	Item No.
<b>Universal Abutment OverdenSURE Attachment</b>	UMUA-ODS





## OverdenSURE® Removable Attachment System

### OverdenSURE® Abutments US Only

Retention Kit ODSZ-RIKIT2001 not included, please order separately.

Implant Platform	Collar Height					
	1.0 mm	2.0 mm	3.0 mm	4.0 mm	5.0 mm	6.0 mm
<span style="color: blue;">●</span> NP (2.9 mmD)	ODSA-NP201	ODSA-NP202	ODSA-NP203	ODSA-NP204	ODSA-NP205	ODSA-NP206
<span style="color: green;">●</span> 3.5 mmD	ODSA-TSV301	ODSA-TSV302	ODSA-TSV303	ODSA-TSV304	ODSA-TSV305	ODSA-TSV306
<span style="color: purple;">●</span> 4.5 mmD	ODSA-TSV401	ODSA-TSV402	ODSA-TSV403	ODSA-TSV404	ODSA-TSV405	ODSA-TSV406



### All markets outside the US

Retention Kit ODS-RIKIT2001 included. Available in all active geographies except the U.S.

Implant Platform	Collar Height					
	1.0 mm	2.0 mm	3.0 mm	4.0 mm	5.0 mm	6.0 mm
<span style="color: blue;">●</span> NP (2.9 mmD)	ODS-NP201	ODS-NP202	ODS-NP203	ODS-NP204	ODS-NP205	ODS-NP206
<span style="color: green;">●</span> 3.5 mmD	ODS-TSV301	ODS-TSV302	ODS-TSV303	ODS-TSV304	ODS-TSV305	ODS-TSV306
<span style="color: purple;">●</span> 4.5 mmD	ODS-TSV401	ODS-TSV402	ODS-TSV403	ODS-TSV404	ODS-TSV405	ODS-TSV406



### OverdenSURE Retention Inserts

#### US only

Description	Item No.
Retention Kit 20° (Qty. 1 Set)	ODSZ-RIKIT2001
Retention Kit 20° (Qty. 2 Sets)	ODSZ-RIKIT2002
Retention Kit 40° (Qty. 1 Set)	ODSZ-RIKIT4001
Retention Kit 40° (Qty. 2 Sets)	ODSZ-RIKIT4002
Blue Retention Insert 20° (Qty. 4)	ODSZ-RIB2004
Pink Retention Insert 20° (Qty. 4)	ODSZ-RIP2004
Clear Retention Insert 20° (Qty. 4)	ODSZ-RIC2004
Red Retention Insert 40° (Qty. 4)	ODSZ-RIR4004
Yellow Retention Insert 40° (Qty. 4)	ODSZ-RIY4004
Green Retention Insert 40° (Qty. 4)	ODSZ-RIG4004



#### All markets outside the US

Description	Item No.
Retention Kit 20° (Qty. 1 Set)	ODS-RIKIT2001
Retention Kit 20° (Qty. 2 Sets)	ODS-RIKIT2002
Retention Kit 40° (Qty. 1 Set)	ODS-RIKIT4001
Retention Kit 40° (Qty. 2 Sets)	ODS-RIKIT4002
Blue Retention Insert 20° (Qty. 4)	ODS-RIB2004
Pink Retention Insert 20° (Qty. 4)	ODS-RIP2004
Clear Retention Insert 20° (Qty. 4)	ODS-RIC2004
Red Retention Insert 40° (Qty. 4)	ODS-RIR4004
Yellow Retention Insert 40° (Qty. 4)	ODS-RIY4004
Green Retention Insert 40° (Qty. 4)	ODS-RIG4004

### OverdenSURE Tools and Accessories

Description	Item No.
Impression Coping (Qty. 1)	ODS-IC01
Impression Coping (Qty. 4)	ODS-IC04
Impression Coping (Qty. 10)	ODS-IC010
Analog (Qty. 1)	ODS-AA01
Analog (Qty. 4)	ODS-AA04
Analog (Qty. 10)	ODS-AA010
Abutment Bar Attachment (Qty. 1)	ODS-BARATT01
Abutment Bar Attachment (Qty. 2)	ODS-BARATT02
Abutment Bar Attachment (Qty. 4)	ODS-BARATT04
Retention Housing Cap (Qty. 1)	ODS-RH01
Retention Housing Cap (Qty. 4)	ODS-RH04
Retention Housing Cap (Qty. 10)	ODS-RH010
Blockout Spacer (Qty. 20)	ODS-BS020
Abutment Driver	ODS-DRVR
Removal and Insertion Tool	ODS-IRTOOL



### Ball Abutments

Abutments do not engage internal hex connection. Includes Cap Attachment Housing and Nylon Liner.  
 NP platform ball abutments do not include cap attachment housing and nylon liner.

Implant Platform	Cuff Height		
	2.0 mm	4.0 mm	6.0 mm
● NP (2.9 mmD)	CBANP2	CBANP4	CBANP6
● 3.5 mmD	BAC2	BAC4	BAC6
● 4.5 mmD	BACW2	BACW4	BACW6



### Ball Abutment Transfer Components

Description	Item No.
Ball Abutment Transfer (Qty. 2)	BAT
Ball Abutment Replica	BAR



### Prosthetic Components

Description	Item No.
Cap Attachment Housing (CAH) / Cap Attachment Nylon Liner (CAN)	CA
Cap Attachment Housing	CAH
Cap Attachment Nylon Liner, Transparent	CAN
Cap Attachment Nylon Liner, Gray — Rigid Retention	CAN-G
Cap Attachment Transfer, Yellow	CAT
Castable Ball Pattern, 2 balls per pattern	CAB
Micro Cap Attachment Nylon Liner	CANM



## Prosthetic Tools

### Torque Wrenches and Ratchets


Description	Item No.
Torque Wrench, Restorative Adjustable torque range 10 Ncm – 35 Ncm	TWR
Low Torque Indicating Ratchet Wrench (Includes C9980 Latchlock Adapter)	L-TIRW
Low Torque Indicating Ratchet Wrench Standard ISO 1797 Latchlock Adapter	C9980
GemLock Retaining Square Ratchet for Restorative Use with HX1.25, HXL1.25 and SRT	RSR

Note: Do not tighten surgical and prosthetic screws beyond the recommended torque indicated in the technique manual and/or IFU.



### Hex Drivers 1.25 mmD for Surgical and Prosthetic Screws

Description	Mode of Use	Item No.
Hex Driver, Short, with GemLock Retention, 1.25 mmD, 22 mmL	Hand	HXGR1.25
Hex Driver, Long, with GemLock Retention, 1.25 mmD, 30 mmL	Hand	HXLGR1.25
Latch-Lock Hex Driver for Surgical and Prosthetic Screws, Short, 1.25 mmD, 23 mmL May require Reduction Handpiece	Handpiece, L-TIRW	HX1.25D
Latch-Lock Hex-Driver for Surgical and Prosthetic Screws, Long, 1.25 mmD, 26 mmL May require Reduction Handpiece	Handpiece, L-TIRW	HXL1.25D
Torque Wrench Hex Driver, Short, 1.25 mmD, 17 mmL	TWR	TW1.25
Torque Wrench Hex Driver, Long, 1.25 mmD, 22 mmL	TWR	TW1.25L
Hex Driver, Short, Standard, 1.25 mmD, 17 mmL	RSR	HX1.25
Hex Driver, Long, Standard, 1.25 mmD, 22 mmL	RSR	HXL1.25

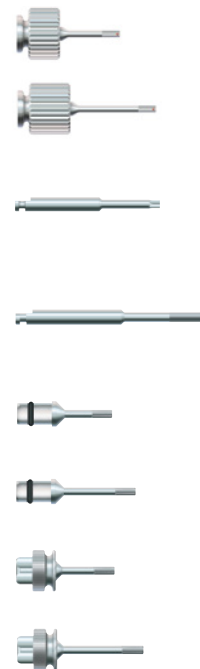

### Prosthetic Tools for Universal Multi-Unit Abutments

Description	Item No.
Universal Abutment Multi-Unit Driver	UMUA-D
ISO Latch, 4x4 Driver	ISO4X4A
Angulated Screw Channel Screwdriver, 24 mm(L)	ASC-SD24
Angulated Screw Channel Screwdriver, 30 mm(L)	ASC-SD30



### Angled Screw Channel Tools and Accessories for Express and Flex Abutments

Description	Mode of Use	Item No.
Angled Screw Channel Driver, 24 mmL	TWR	TASCD24
Angled Screw Channel Driver, 30 mmL	TWR	TASCD30
Angled Screw Channel Driver Tip, 24 mmL	L-TIRW	TASCT24
Angled Screw Channel Driver Tip, 30 mmL	L-TIRW	TASCT30



### Removal Tools

Description	Mode of Use	Item No.
Removal Tool for NP (2.9 mmD) Abutments	Hand or RSR	CLRT2
Removal Tool for Internal Hex Implant Abutments Included in TSV Surgical Kits TSVKIT and STRKIT	Hand or RSR	TLRT2
Removal Tool for Abutment Screws or Fixation Screws with 1.25 mmD Hex, Carbide Steel Note: Do not autoclave	RSR	SRT



### Additional Prosthetic Tools and Accessories



Description	Item No.
Prosthetic Kit Tray, Autoclavable, empty	2320
Abutment Holder Requires Implant Analog to attach abutments	ABTH




# Surgical Kits and Instrumentation

## TSV Surgical Kit Layout Chart for TSX Implant Placement - Driva™ Gold Series Drills

### Tapered Screw-Vent Surgical Kit (TSVKITG)

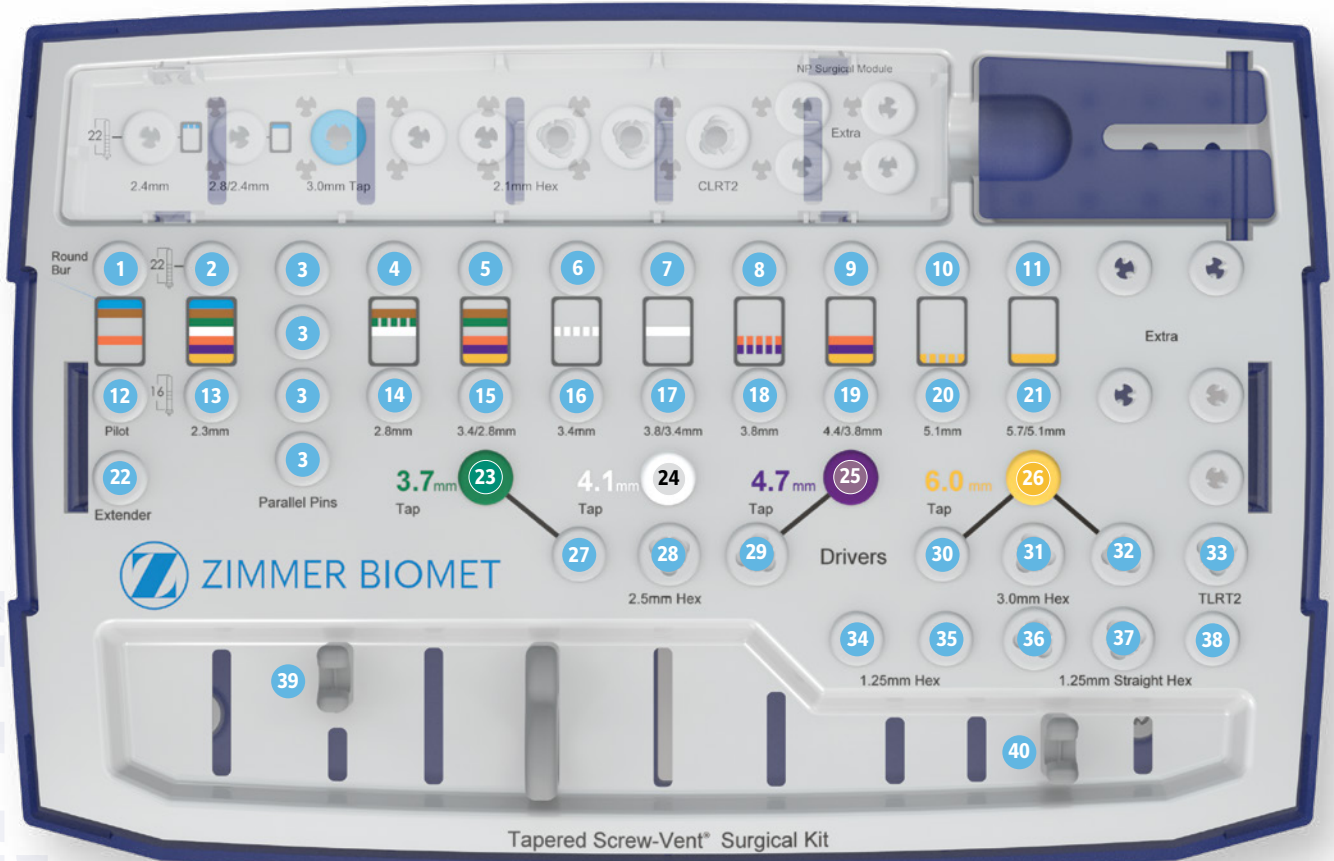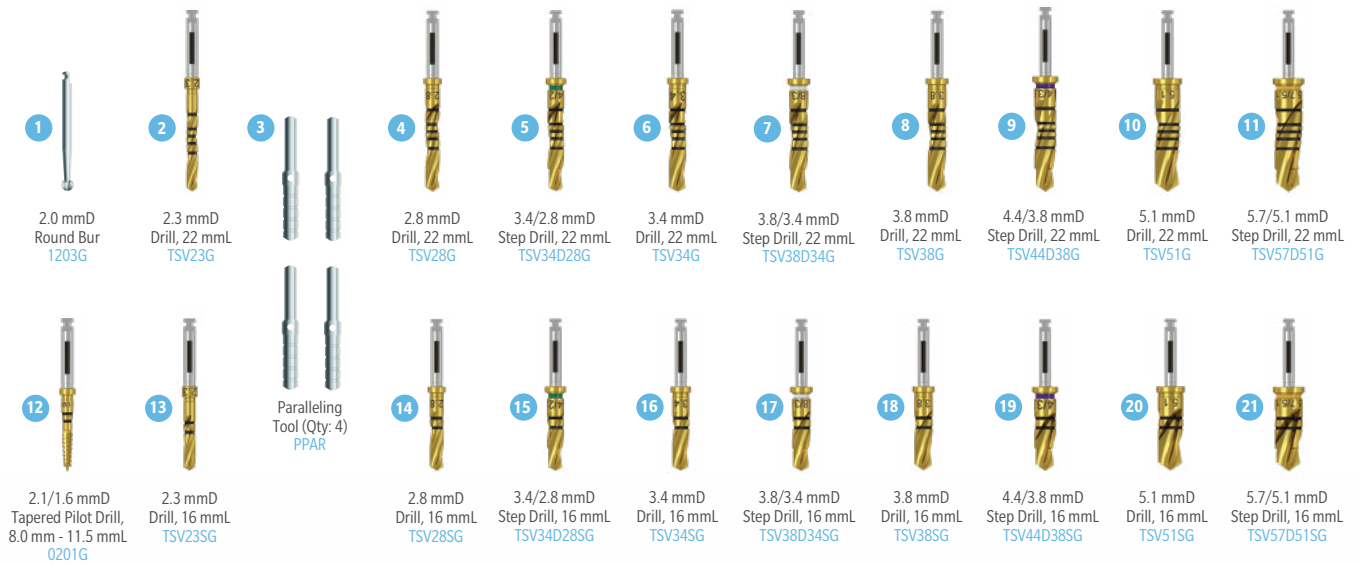


**NOTE: TSV Taps not utilized with TSX Implant**

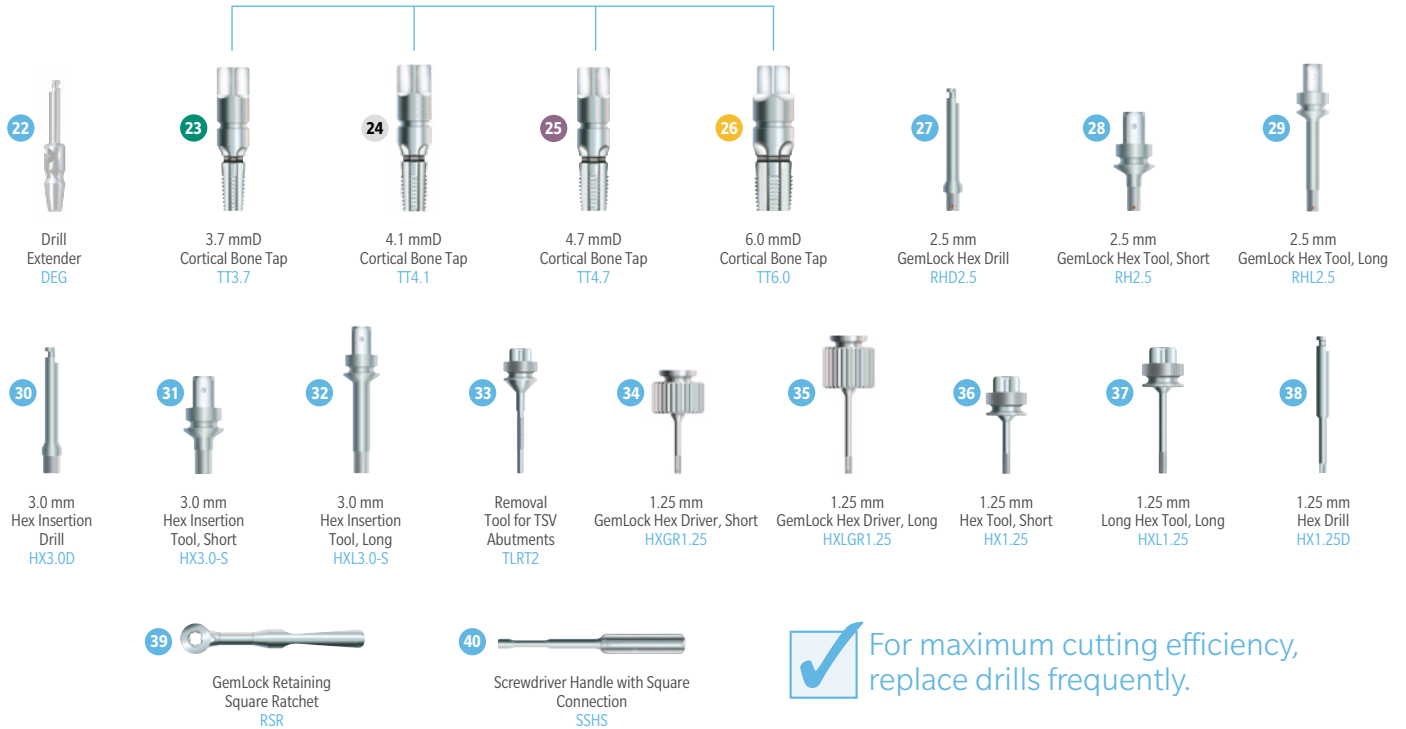

 For maximum cutting efficiency, replace drills frequently.

## NP Surgical Module for 3.1 mmD TSX Implant (NPMODG)

**NOTE: NPMODG Tap not used with TSX Implant**

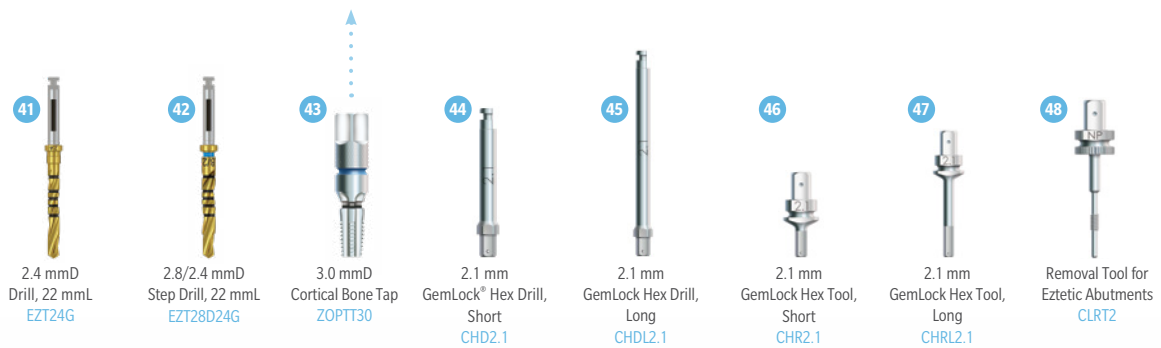

The NP Surgical Module snaps into the Surgical Kit

## Tapered Screw-Vent Surgical Kit for TSX Implants

### Tapered Screw-Vent Surgical Kit, Complete

Description	Item No.
<b>Tapered Screw-Vent Surgical Kit</b> For placement of 3.7 mmD, 4.1 mmD, 4.7 mmD, and 6.0 mmD TSX, Trabecular Metal® and Tapered Screw-Vent Implants	<b>TSVKITG</b>
<b>TSV Surgical Tray, Empty</b>	TSVTRAYG
2.1/1.6 mmD Tapered Pilot Drill, 8 mmL - 11.5 mmL	0201G
2.0 mmD Round Bur	1203G
2.3 mmD Driva™ Gold Series Drill, 16 mmL	TSV23SG
2.3 mmD Driva Gold Series Drill, 22 mmL	TSV23G
2.8 mmD Driva Gold Series Drill, 16 mmL	TSV28SG
2.8 mmD Driva Gold Series Drill, 22 mmL	TSV28G
3.4/2.8 mmD Driva Gold Series Step Drill, 16 mmL	TSV34D28SG
3.4/2.8 mmD Driva Gold Series Step Drill, 22 mmL	TSV34D28G
3.4 mmD Driva Gold Series Drill, 16 mmL	TSV34SG
3.4 mmD Driva Gold Series Drill, 22 mmL	TSV34G
3.8/3.4 mmD Driva Gold Series Step Drill, 16 mmL	TSV38D34SG
3.8/3.4 mmD Driva Gold Series Step Drill, 22 mmL	TSV38D34G
3.8 mmD Driva Gold Series Drill, 16 mmL	TSV38SG
3.8 mmD Driva Gold Series Drill, 22 mmL	TSV38G
4.4/3.8 mmD Driva Gold Series Step Drill, 16 mmL	TSV44D38SG
4.4/3.8 mmD Driva Gold Series Step Drill, 22 mmL	TSV44D38G
5.1 mmD Driva Gold Series Drill, 16 mmL	TSV51SG
5.1 mmD Driva Gold Series Drill, 22 mmL	TSV51G
5.7/5.1 mmD Driva Gold Series Step Drill, 16 mmL	TSV57D51SG
5.7/5.1 mmD Driva Gold Series Step Drill, 22 mmL	TSV57D51G
3.7 mmD Cortical Bone Tap Tool	TT3.7
4.1 mmD Cortical Bone Tap Tool	TT4.1
4.7 mmD Cortical Bone Tap Tool	TT4.7
6.0 mmD Cortical Bone Tap Tool	TT6.0
1.25 mmD Hex Driver, Short, with GemLock Retention, 22 mmL	HXGR1.25
1.25 mmD Hex Driver, Long, with GemLock Retention, 30 mmL	HXLGR1.25
1.25 mmD Hex Driver, Short, 17 mmL	HX1.25
1.25 mmD Hex Driver, Long, 22 mmL	HXL1.25
1.25 mmD Latch-Lock Hex Driver, 23 mmL	HX1.25D
2.5 mmD GemLock Retaining Hex Driver, Short, 17 mmL	RH2.5
2.5 mmD GemLock Retaining Hex Driver, Long, 28 mmL	RHL2.5
2.5 mmD GemLock Retaining Hex Driver, 21 mmL	RHD2.5
3.0 mmD Hex Driver, Short, 17 mmL*	HX3.0-S
3.0 mmD Hex Driver, Long, 28 mmL*	HXL3.0-S
3.0 mmD Hex Driver, 25 mmL*	HX3.0D
Drill Extender	DEG
Paralleling Tool (Qty. 4)	PPAR
GemLock Retaining Square Ratchet	RSR
Screwdriver Handle with Square Connection	SSHS
Removal Tool for Internal Hex Implant Abutments	TLRT2
Tapered Screw-Vent Staging Block	TSVBLKG



NOTE: Drills marked in blue are included in TSVTRAYDG on page 25.

\*3.0 mmD Hex Drivers not utilized with TSX Implant.



## Tapered Screw-Vent Surgical Kit, Partial Configurations

Description	Item No.
Tapered Screw-Vent Starter Kit For placement of 3.7 mmD and 4.7 mmD Implants only	STRKITG
2.1/1.6 mmD Drill, 8 mmL - 11.5mmL	0201G
2.3 mmD Driva Gold Series Surgical Drill, Instrument Kit System, 22 mmL	TSV23G
2.8 mmD Driva Gold Series Surgical Drill, Instrument Kit System, 22 mmL	TSV28G
3.4/2.8 mmD Driva Gold Series Surgical Step Drill, Instrument Kit System, 22 mmL	TSV34D28G
3.8 mmD Driva Gold Series Surgical Drill, Instrument Kit System, 22 mmL	TSV38G
4.4/3.8 mmD Driva Gold Series Surgical Step Drill, Instrument Kit System, 22 mmL	TSV44D38G
1.25 mmD Hex Driver, Short, with GemLock Retention, 22 mmL	HXGR1.25
1.25 mmD Hex Driver, Long, with GemLock Retention, 30 mmL	HXLGR1.25
1.25 mmD Hex Driver, Short, 17 mmL	HX1.25
2.5 mmD GemLock Retaining Hex Driver, Long, 28 mmL	RHL2.5
2.5 mmD GemLock Retaining Hex Driver, 21 mmL	RHD2.5
Drill Extender	DEG
Paralleling Tool (Qty. 4)	PPAR
GemLock Retaining Square Ratchet	RSR
Screwdriver Handle with Square Connection	SSHS
Removal Tool for Internal Hex Implant Abutments	TLRT2
3.7 mmD Cortical Bone Tap Tool	TT3.7
4.7 mmD Cortical Bone Tap Tool	TT4.7
Tapered Screw-Vent Staging Block	TSVBKLG
TSV Surgical Tray, Empty	TSVTRAYG
Surgical Tray and Drills for Trabecular Metal and Tapered Screw-Vent Implants <a href="#">Includes TSVTRAYG, TSVBLKG and drills marked in blue on page 24</a>	TSVTRAYDG
Tapered Screw-Vent Staging Block Block only	TSVBKLG



## NP Surgical Module

Description	Item No.
NP Surgical Module (To be inserted into TSVKITG). Includes: (Qty. 1)	NPMODG
NP Surgical Module (Tray Only) (Qty.1)	NPTRAYG
2.4 mmD Driva™ Drill, 22 mmL (Qty.1)	EZT24G
2.8/2.4 mmD Driva Step Drill, 22 mmL (Qty.1)	EZT28D24G
3.0 mmD Cortical Bone Tap Tool (Qty.1)	ZOPTT30
2.1 mm GemLock Hex Drill, Latch Lock, Short (Qty.1)	CHD2.1
2.1 mm GemLock Hex Drill, Latch Lock, Long (Qty.1)	CHDL2.1
2.1 mm GemLock Hex Tool, Ratchet, Short (Qty.1)	CHR2.1
2.1 mm GemLock Hex Tool, Ratchet, Long (Qty.1)	CHRL2.1
Removal Tool for Eztetic Abutments (Qty.1)	CLRT2



## Dríva Gold Series Surgical Drills and Drill Stops

### Surgical Pilot Drills

Diameter	15 mmL*	16 mmL*	19 mmL	22 mmL*	25 mmL
2.1/1.6 mmD	0201G	—	—	—	—




### Dríva Dríva Surgical Drills

Diameter	15 mmL*	16 mmL*	19 mmL	22 mmL*	25 mmL
2.3 mmD	—	TSV23SG	STR23D19	TSV23G	STR23D25
2.4 mmD	—	—	—	EZT24G	—
2.8 mmD	—	TSV28SG	STR28D19	TSV28G	STR28D25
3.4 mmD	—	TSV34SG	STR34D19	TSV34G	STR34D25
3.8 mmD	—	TSV38SG	STR38D19	TSV38G	STR38D25
4.4 mmD	—	TSV44SG	—	TSV44G	—
5.1 mmD	—	TSV51SG	—	TSV51G	—



### Dríva Surgical Step Drills


Diameter	16 mmL*	19 mmL	22 mmL*	25 mmL	Color Code	
2.8/2.4 mmD	—	—	EZT28D24G	—	—	—
3.4/2.8 mmD	TSV34D28SG	STP34D19	TSV34D28G	STP34D25	Green	●
3.8/3.4 mmD	TSV38D34SG	STP38D19	TSV38D34G	STP38D25	White	○
4.4/3.8 mmD	TSV44D38SG	STP44D19	TSV44D38G	STP44D25	Purple	●
5.1/4.4 mmD	TSV51D44SG**	—	TSV51D44G**	—	Black	●
5.7/5.1 mmD	TSV57D51SG	—	TSV57D51G	—	Yellow	●



\*The 15 mmL, 16 mmL and 22 mmL Drills feature axial stripes to help identify use with the Drill Stop Kit.

\*\*TSV51D44SG and TSV51D44G are the final drills for the 5.4 mmD TSX Implant in dense bone, are optional interim drills in the 6.0 mmD drilling sequence and are sold separately and not in surgical kits.

The depth markings are machined and laser-etched for increased visibility.  
 The bands are located approximately 1.25 mm longer than the implant-abutment junction.  
 (For example: the 13 mm band is dimensioned 14.25 mm from the tip of the drill).

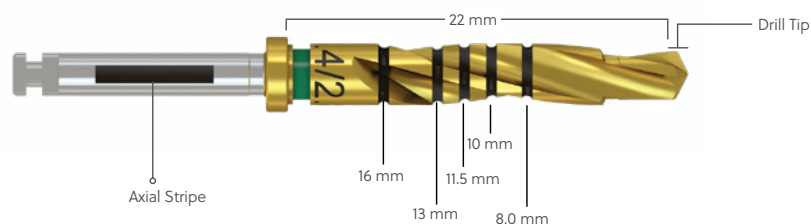


## Single-Patient Drills

Description	Contents	Item No.
Drill Kit, Single-Patient, Long 3.7 mmD Implant, 17 mmL	Round Bur 2.3 mmD Pilot Drill 3.4/2.8 mmD Step Drill	DSTK3
Drill Kit, Single-Patient, Short 3.7 mmD Implant, 11 mmL	Round Bur 2.3 mmD Pilot Drill 3.4/2.8 mmD Step Drill	DSTK3S
Drill, Single-Patient, Long 4.7 mmD Implant, 17 mmL	4.4/3.8 mmD Step Drill	DST4
Drill, Single-Patient, Short 4.7 mmD Implant, 11 mmL	4.4/3.8 mmD Step Drill	DST4S
Drill, Single-Patient, Long 6.0 mmD Implant, 17 mmL	5.7/5.1 mmD Step Drill	DST6
Drill, Single-Patient, Short 6.0 mmD Implant, 11 mmL	5.7/5.1 mmD Step Drill	DST6S

Note: No internal irrigation. Kits with long drills have depth markings for 8, 10, 11.5, 13, and 16 mmL implants. Kits with short drills have depth markings for 8 and 10 mmL implants.


## Implant Placement Instruments

Description	Item No.
High Torque Indicating Ratchet Wrench	ZTIRW
GemLock Retaining Square Ratchet	RSR
Stainless Steel Screwdriver Handle	SSHS




## Hex Drivers 1.25 mmD

Description	Mode of Use	Item No.
Hex Driver, Short, with GemLock Retention, 1.25 mmD, 22 mmL	Hand	HXGR1.25
Hex Driver, Long, with GemLock Retention, 1.25 mmD, 30 mmL	Hand	HXLGR1.25
Latch-Lock Hex Driver for Surgical and Prosthetic Screws, Short, 1.25 mmD, 23 mmL May require Reduction Handpiece	Handpiece, L-TIRW	HX1.25D
Latch-Lock Hex-Driver for Surgical and Prosthetic Screws, Long, 1.25 mmD, 26 mmL May require Reduction Handpiece	Handpiece, L-TIRW	HXL1.25D
Hex Driver, Short, Standard, 1.25 mmD, 17 mmL	RSR	HX1.25
Hex Driver, Long, Standard, 1.25 mmD, 22 mmL	RSR	HXL1.25

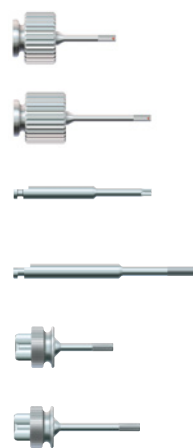

### Hex Drivers 2.1 mmD for 3.1 mmD TSX Implant Placement

Description	Mode of Use	Item No.
2.1 mm GemLock Hex Tool, Ratchet, Short	ZTIRW, RSR, SSHS	CHR2.1
2.1 mm GemLock Hex Tool, Ratchet, Long	ZTIRW, RSR, SSHS	CHRL2.1
2.1 mm GemLock Hex Drill, Latch-Lock, Short	Handpiece	CHD2.1
2.1 mm GemLock Hex Drill, Latch-Lock, Long	Handpiece	CHDL2.1



### Hex Drivers 2.5 mmD for 3.7 to 6.0 mmD TSX Implant Placement

Description	Mode of Use	Item No.
2.5 mm Hex Driver with GemLock Retention, Short, 17 mmL	ZTIRW, RSR, SSHS	GHX2.5
2.5 mm Hex Driver with GemLock Retention, Long, 28 mmL	ZTIRW, RSR, SSHS	GHX2.5L
2.5 mm Latch-lock Hex Driver with GemLock Retention, Short, 21 mmL	Handpiece	GHX2.5D
2.5 mm Latch-lock Hex Driver with GemLock Retention, Long, 30 mmL	Handpiece	GHX2.5DL



### Surgical Instruments

Description	Item No.
Drill Extender	DEG
Paralleling Tool	PPAR
Round Bur	1203G
Removal Tool for Screw-Type Implants, Carbide Steel Note: Do not autoclave	IRT



## Guided Surgery Instrumentation

TSX implants can be placed in a fully-guided fashion utilizing the RealGUIDE Z3D Guided Surgery Kit and instrumentation shown on pages 27-28. Information on the partially-guided surgical module for TSVKITG can be found on page 29.

### Fully Guided RealGUIDE™ Z3D Guided Surgery Kit\*

Product	Item No.
RealGUIDE Kit Z3D Surgical Kit (fully loaded)	3DM0070ZUS
Autoclavable Kit RealGUIDE Z3D Box	3DM00616ZUS

\*Not approved in all markets.



### Configuration

Product	Item No.
<b>Drill for Fixation Pin</b> max. 1,000 rpm, hardened stainless steel AISI 420B with DLC coating	3DM00610ZUS
<b>Fixation Pin</b> TiAl6V4 ASTM F136	3DM00609ZUS
<b>Torque Wrench Extension</b> max. 50 Ncm, hardened stainless steel AISI 420F MOD	3DM00623ZUS
<b>4 × 4 Square Connector for handpiece</b> max. 50 Ncm, hardened stainless steel AISI 420F MOD	3DM00612ZUS
<b>Mouth Opening Gauge / Bite Gauge</b> hardened stainless steel AISI 303	3DM00622ZUS
<b>Mucotome / Tissue Punch</b> Internal diameter: 4.2 mm, max. 100 rpm, hardened stainless steel AISI 420F MOD with DLC coating	3DM00607ZUS
<b>Bone Crest Leveler</b> max. 600 rpm, hardened stainless steel AISI 420B with DLC coating	3DM00614ZUS
<b>Start Drill</b> Implant site preparation drill, max. 600 rpm, hardened stainless steel AISI 420B with DLC coating	3DM00621ZUS
<b>Drill 2.4 × 6 mmD</b> max. 800 rpm, hardened stainless steel AISI 420B with DLC coating	3DM00619ZUS
<b>TSX Z3D Staging Tool</b> Long for 11.5/13/16 mmL Implants	3DM00633ZIML
<b>TSX Z3D Staging Tool</b> Short for 8/10 mmL Implants	3DM00633ZIMS



## Fully Guided Z3D Kit Components

### RealGUIDE Z3D Implant Mounts (hardened stainless steel AISI 420F MOD)

Product	Item No.
ZimVie TSX /Eztetic 3.1mmD incl. screw, max. 20 rpm, 50 Ncm	3DM00606ZIM31US
ZimVie TSX 3.7/4.1/4.7 mmD, ZimVie TSV 3.7/4.1 mmD incl. screw, max. 20 rpm, 50 Ncm	3DM00606ZIM35US
ZimVie TSV 4.7 mmD incl. screw, max. 20 rpm, 50 Ncm	3DM00606ZIM47US



### RealGUIDE Z3D Drills (hardened stainless steel AISI 420B with DLC coating)

Length	Drill 2.4 mmD	Double Diameter Drill 2.8 / 2.4 mmD	Double Diameter Drill 3.4 / 2.8 mmD	Double Diameter Drill 3.8 / 3.4 mmD	Double Diameter Drill 4.4 / 3.8 mmD
	max. 800 rpm				
					
8 mm	3DM00613.24.080ZUS	3DM00613.28.080ZUS	3DM00613.34.080ZUS	3DM00613.38.080ZUS	3DM00613.44.080ZUS
10 mm	3DM00613.24.100ZUS	3DM00613.28.100ZUS	3DM00613.34.100ZUS	3DM00613.38.100ZUS	3DM00613.44.100ZUS
11.5 mm	3DM00613.24.115ZUS	3DM00613.28.115ZUS	3DM00613.34.115ZUS	3DM00613.38.115ZUS	3DM00613.44.115ZUS
13 mm	3DM00613.24.130ZUS	3DM00613.28.130ZUS	3DM00613.34.130ZUS	3DM00613.38.130ZUS	3DM00613.44.130ZUS
16 mm	3DM00613.24.160ZUS	3DM00613.28.160ZUS	3DM00613.34.160ZUS	3DM00613.38.160ZUS	3DM00613.44.160ZUS

### RealGUIDE Z3D Surgical Guide Accessories

Product	Item No.
Surgical Guide Sleeve RG CAD Procedure 5.05 mm, compatible 3DM RG, Zimmer Biomet Z3D, Nobel RP Kit (10 pcs)	3DM00670
Surgical Guide Pin Fixation Sleeve RG CAD Procedure (10 pcs)	3DM00671

## Partially Guided Surgery Instrumentation

Description	Item No.
<b>Guided Surgery Drill Module</b> Can be inserted into the TSVKITG for an all-in-one Guided Surgery Kit	GSMOD
2.3 mmD Driva EG Surgical Drill, 19 mmL	STR23D19
2.3 mmD Driva EG Surgical Drill, 25 mmL	STR23D25
2.8/2.4 mmD Driva EG Surgical Step Drill, 19 mmL	STP28D19
2.8/2.4 mmD Driva EG Surgical Step Drill, 25 mmL	STP28D25
2.8 mmD Driva EG Surgical Drill, 19 mmL	STR28D19
2.8 mmD Driva EG Surgical Drill, 25 mmL	STR28D25
3.4/2.8 mmD Driva EG Surgical Step Drill, 19 mmL	STP34D19
3.4/2.8 mmD Driva EG Surgical Step Drill, 25 mmL	STP34D25
3.4 mmD Driva EG Surgical Drill, 19 mmL	STR34D19
3.4 mmD Driva EG Surgical Drill, 25 mmL	STR34D25
3.8/3.4 mmD Driva EG Surgical Step Drill, 19 mmL	STP38D19
3.8/3.4 mmD Driva EG Surgical Step Drill, 25 mmL	STP38D25
3.8 mmD Driva EG Surgical Drill, 19 mmL	STR38D19
3.8 mmD Driva EG Surgical Drill, 25 mmL	STR38D25
4.4/3.8 mmD Driva EG Surgical Step Drill, 19 mmL	STP44D19
4.4/3.8 mmD Driva EG Surgical Step Drill, 25 mmL	STP44D25



Can be inserted into Tapered Screw-Vent Surgical Kit (TSVKITG)



Guided Surgery Module Insert (Empty)	GSTRAY
--------------------------------------	--------



<b>Tube Adapter Kit*</b> Includes 1 of each Tube Adapter listed below; EG Drills are used with Tube Adapter Kit;	TADKIT
2.3 mmD Tube Adapter, A	TAD23A
2.8 mmD Tube Adapter, A	TAD28A
3.4 mmD Tube Adapter, A	TAD34A
2.3 mmD Tube Adapter, B	TAD23B
2.8 mmD Tube Adapter, B	TAD28B
3.4 mmD Tube Adapter, B	TAD34B
3.8 mmD Tube Adapter, B	TAD38B
4.4 mmD Tube Adapter, B	TAD44B



\* For use with Driva EG Drills and Driva Drills with axial stripe.

## Drill Stop Kit\*

Description	Item No.
<b>Complete Drill Stop Kit</b> Drills not included	DSKIT
Stop Set, 8.0 mmL Implant, 2.3 - 4.4/3.8 mmD x 17/22 mmL Driva Drill (Qty. 5)	SS8D22
Stop Set, 10 mmL Implant, 2.3 - 4.4/3.8 mmD x 17/22 mmL Driva Drill (Qty. 5)	SS10D22
Stop Set, 11.5 mmL Implant, 2.3 - 4.4/3.8 mmD x 17/22 mmL Driva Drill (Qty. 5)	SS11D22
Stop Set, 13 mmL Implant, 2.3 - 4.4/3.8 mmD x 17/22 mmL Driva Drill (Qty. 5)	SS13D22
Stop Set, 8 mmL Implant, 2.3 - 4.4/3.8 mmD x 11/16 mmL Driva Drill (Qty. 5)	SS8D16
Stop Set, 10 mmL Implant - 11/16 mmL Driva Drill and 16 mmL Implant - 17/22 mmL Driva Drill, 2.3 - 4.4/3.8 mmD Driva Drill (Qty. 5)	SS10D16
Stop Set, 11.5 mmL Implant, 2.3 - 4.4/3.8 mmD x 11/16 mmL Driva Drill (Qty. 5)	SS11D16
Stop Set, 8-16 mmL Implant, 5.1 mmD x 11/16 mmL & 17/22 mmL Driva Drill (Qty. 7)	SS51D
Stop Set, 8-16 mmL Implant, 5.7/5.1 mmD x 11/16 mmL & 17/22 mmL Driva Drill (Qty. 7)	SS57D
Drill Stop Multi-Tool	MTL










Tapered Screw-Vent Surgical Kit

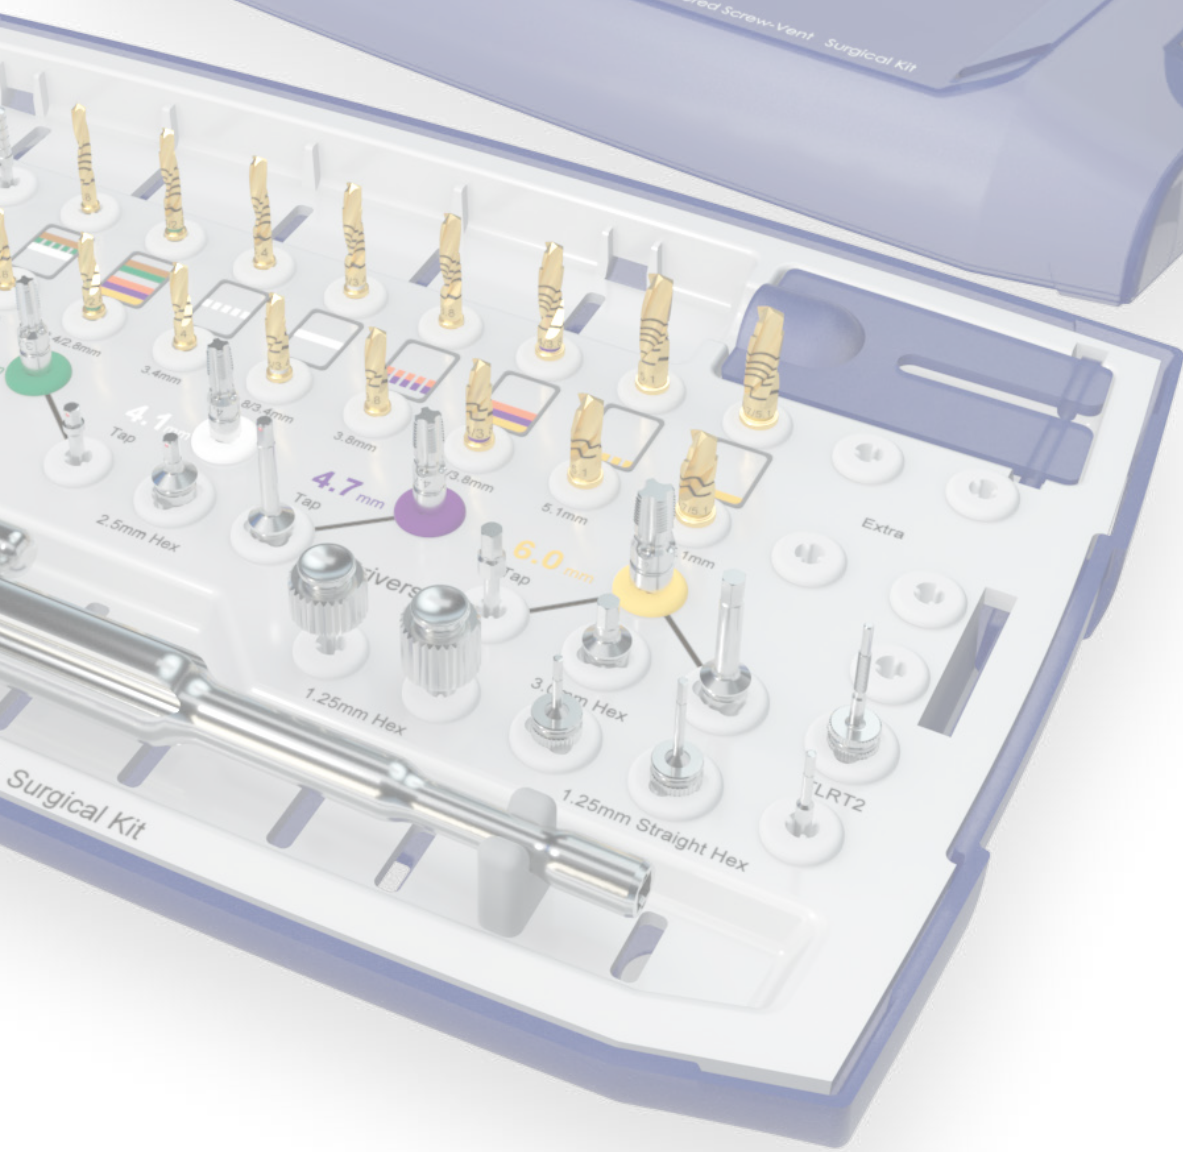

Surgical Kit

Drivers

Extra

LRT2





For more information, visit [ZimVie.com](https://www.zimvie.com)

**ZimVie**  
4555 Riverside Drive  
Palm Beach Gardens, FL 33410  
Phone: +1-561-776-6700  
Fax: +1-561-776-1272



Unless otherwise indicated, as referenced herein, all trademarks and intellectual property rights are the property of ZimVie Inc. or an affiliate; and all products are manufactured by one or more of the dental subsidiaries of ZimVie Inc. (Biomet 3i, LLC, Zimmer Dental, Inc., etc.) and marketed and distributed by ZimVie Dental and its authorized marketing partners. Digital Implant Analogs, Universal Multi-Unit Abutments and OverdenSURE Abutments are manufactured by Terrats Medical S.L. ZTIRW High Torque Indicating Ratchet Wrench and L-TIRW Low Torque Indicating Ratchet Wrench are manufactured by Elos Medtech Pinol A/S. For additional product information, please refer to the individual product labeling or instructions for use. Product clearance and availability may be limited to certain countries/regions. This material is intended for clinicians only and does not comprise medical advice or recommendations. Distribution to any other recipient is prohibited. This material may not be copied or reprinted without the express written consent of ZimVie.

ZVINST0019 REV D 04/24 ©2024 ZimVie. All rights reserved.

